

# INSTRUCTION MANUAL



## CS105/CS105MD Barometric Pressure Sensor

Revision: 3/07



Copyright © 1995-2007  
Campbell Scientific, Inc.

## WARRANTY AND ASSISTANCE

This equipment is warranted by CAMPBELL SCIENTIFIC (CANADA) CORP. ("CSC") to be free from defects in materials and workmanship under normal use and service for **twelve (12) months** from date of shipment unless specified otherwise. \*\*\*\*\* **Batteries are not warranted.** \*\*\*\*\* CSC's obligation under this warranty is limited to repairing or replacing (at CSC's option) defective products. The customer shall assume all costs of removing, reinstalling, and shipping defective products to CSC. CSC will return such products by surface carrier prepaid. This warranty shall not apply to any CSC products which have been subjected to modification, misuse, neglect, accidents of nature, or shipping damage. This warranty is in lieu of all other warranties, expressed or implied, including warranties of merchantability or fitness for a particular purpose. CSC is not liable for special, indirect, incidental, or consequential damages.

Products may not be returned without prior authorization. To obtain a Return Merchandise Authorization (RMA), contact CAMPBELL SCIENTIFIC (CANADA) CORP., at (780) 454-2505. An RMA number will be issued in order to facilitate Repair Personnel in identifying an instrument upon arrival. Please write this number clearly on the outside of the shipping container. Include description of symptoms and all pertinent details.

CAMPBELL SCIENTIFIC (CANADA) CORP. does not accept collect calls.

Non-warranty products returned for repair should be accompanied by a purchase order to cover repair costs.



**CAMPBELL SCIENTIFIC**  
C A N A D A C O R P .

11564 - 149 street - edmonton - alberta - T5M 1W7  
tel 780.454.2505 fax 780.454.2655

[www.campbellsci.ca](http://www.campbellsci.ca)

# CS105/CS105MD Table of Contents

---

*PDF viewers note: These page numbers refer to the printed version of this document. Use the Adobe Acrobat® bookmarks tab for links to specific sections.*

<b>1. General</b> .....	1
<b>2. Specifications</b> .....	1
<b>3. Installation and Wiring</b> .....	2
<b>4. Programming</b> .....	6
4.1 CS105MD .....	6
4.2 CS105 .....	6
<b>5. Long Lead Lengths</b> .....	9
<b>6. Correcting Pressure to Sea Level</b> .....	11
<b>7. Maintenance</b> .....	11

## ***Appendix***

<b>A. Daily Average</b> .....	A-1
-------------------------------	-----

## ***Figures***

1. CS105 Mounted on the Backplate of an ENC12/14 Enclosure, and Connected to a CR1000 Datalogger .....	3
2. CS105MD Mounted on the Backplate of MetData1 Enclosure.....	3
3. CS105 Wiring Diagram .....	4
4. CS105MD Wiring Diagram.....	5

## ***Tables***

1. Signal and Ground Connectors for CS105 .....	4
2. Conversion Factors for Alternative Pressure Units .....	6



# CS105/CS105MD Barometric Pressure Sensor

---

## 1. General

The CS105 analog barometer uses Vaisala's Barocap® silicon capacitive pressure sensor. The Barocap sensor has been designed for accurate and stable measurement of barometric pressure. The CS105 outputs a linear 0 to 2.5 VDC signal that corresponds to 600 to 1060 mb. It can be operated in a powerup or continuous mode. In the powerup mode the datalogger switches 12 VDC power to the barometer during the measurement. The datalogger then powers down the barometer between measurements to conserve power.

## 2. Specifications

### Operating Range

Pressure: 600 mb to 1060 mb  
Temperature: -40°C to +60°C  
Humidity: non-condensing

### Accuracy

Total Accuracy\*\*\*  
±0.5 mb @ +20°C  
±2 mb @ 0°C to +40°C  
±4 mb @ -20°C to +45°C  
±6 mb @ -40°C to +60°C  
Linearity\*: ±0.45 mb @ 20°C  
Hysteresis\*: ±0.05 mb @ 20°C  
Repeatability\*: ±0.05 mb @ 20°C  
Calibration uncertainty\*\*: ±0.15 mb @ 20°C  
Long-Term Stability: ±0.1 mb per year

\* Defined as ±2 standard deviation limits of end-point non-linearity, hysteresis error, or repeatability error

\*\* Defined as ±2 standard deviation limits of inaccuracy of the working standard at 1000 mb in comparison to international standards (NIST)

\*\*\* Defined as the root sum of the squares (RSS) of end-point non-linearity, hysteresis error, repeatability error and calibration uncertainty at room temperature

### General

Dimensions: 9.7 cm x 5.9 cm x 2.1 cm (3.8" x 2.3" x 0.8")

Weight: 110 g (4 oz)

Housing material: anodized aluminum

Supply Voltage: 10 to 30 VDC

Supply Voltage Control: When enabled with an internal jumper, the CS105 is on continually. When disabled, the CS105 can be turned on/off with 5 VDC/0 VDC.

Supply voltage sensitivity: Less than 0.1 mb

Current Consumption: <4 mA (active); <1  $\mu$ A (quiescent)

Output Voltage: 0 to 2.5 VDC

Warm Up Time: 1 second

Pressure fitting: barbed fitting for 1/8" I.D. tubing

Overpressure limit: 2000 mb

---

**NOTE** The black outer jacket of the cable is Santoprene<sup>®</sup> rubber. This compound was chosen for its resistance to temperature extremes, moisture, and UV degradation. However, this jacket will support combustion in air. It is rated as slow burning when tested according to U.L. 94 H.B. and will pass FMVSS302. Local fire codes may preclude its use inside buildings.

---

### 3. Installation and Wiring

The CS105 can be operated in one of two modes: powerup and continuous. The mode is selected by a jumper located underneath a black plug on the face of the barometer. When the jumper is not installed, the CS105 is in powerup mode and the datalogger turns the CS105 on and off with a control port or excitation channel; to use the excitation channel the datalogger must be able to provide an excitation voltage of 5 VDC. When the jumper is installed the CS105 is powered continuously.

---

**NOTE** CS105s shipped from Campbell Scientific are configured for powerup mode (jumper open).

---

---

**NOTE** CS105MDs shipped from Campbell Scientific are configured for continuous power mode (jumper closed).

---

Mount the CS105 to the backplate in the same enclosure that the datalogger is located in (Figures 1 and 2).

---

**NOTE** On the older (grey jacketed) cable pressure (VOUT) was brown and signal ground (AGND) was white.

---

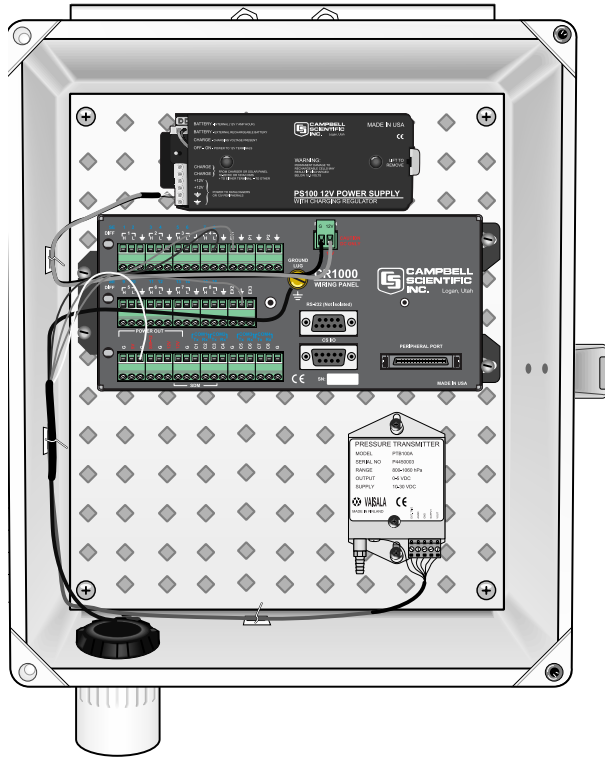


FIGURE 1. CS105 Mounted on the Backplate of an ENC12/14 Enclosure, and Connected to a CR1000 Datalogger

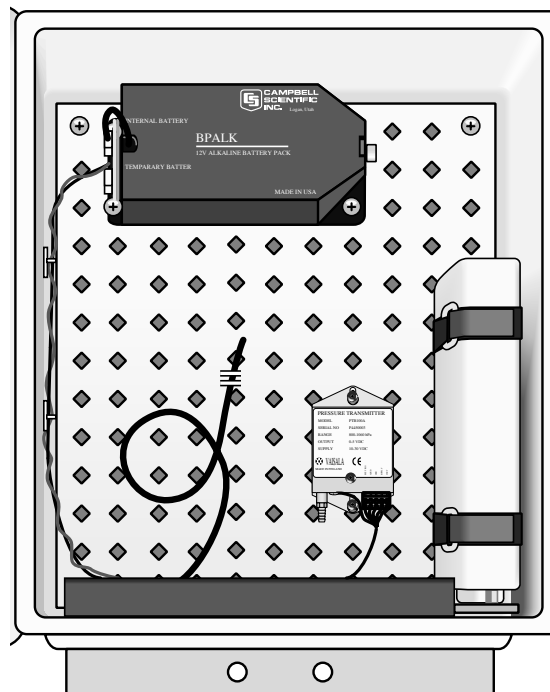


FIGURE 2. CS105MD Mounted on the Backplate of MetData1 Enclosure

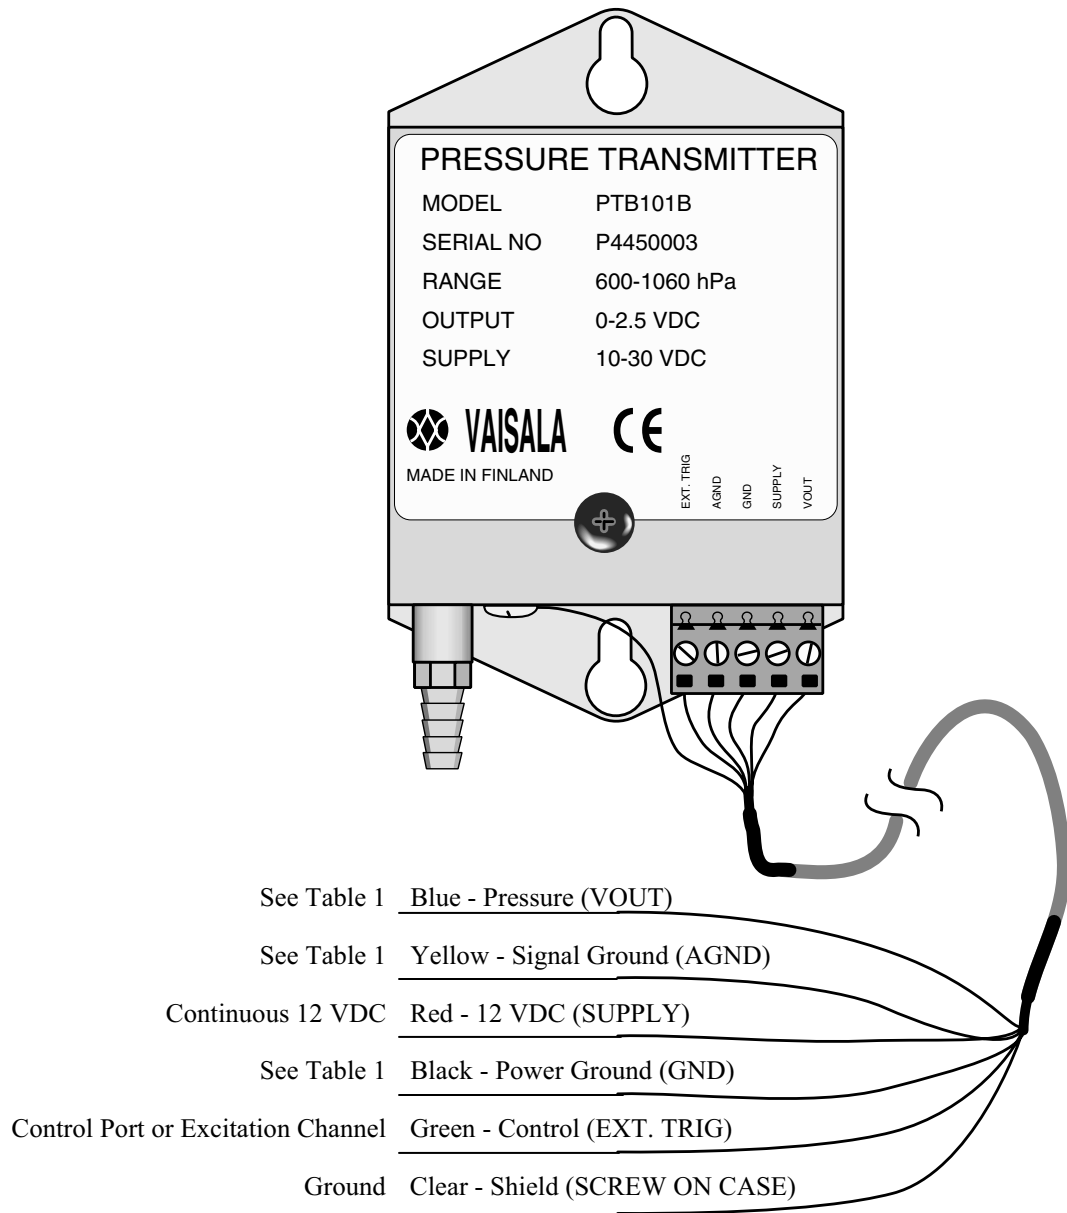


FIGURE 3. CS105 Wiring Diagram

TABLE 1. Signal and Ground Connectors for CS105		
	Single-Ended Measurement	Differential Measurement
Blue	S.E. Input, S.E. 7 (4H)	High Side of Diff Input (4H)
Yellow	AG (CR10(X), CR500, CR510) ⊕ (Other Dataloggers)	Low Side of Diff. Input (4L)
Black	⊕ (21X, CR7, CR9000(X)) G (Other Dataloggers)	⊕ (21X, CR7, CR9000(X)) G (Other Dataloggers)

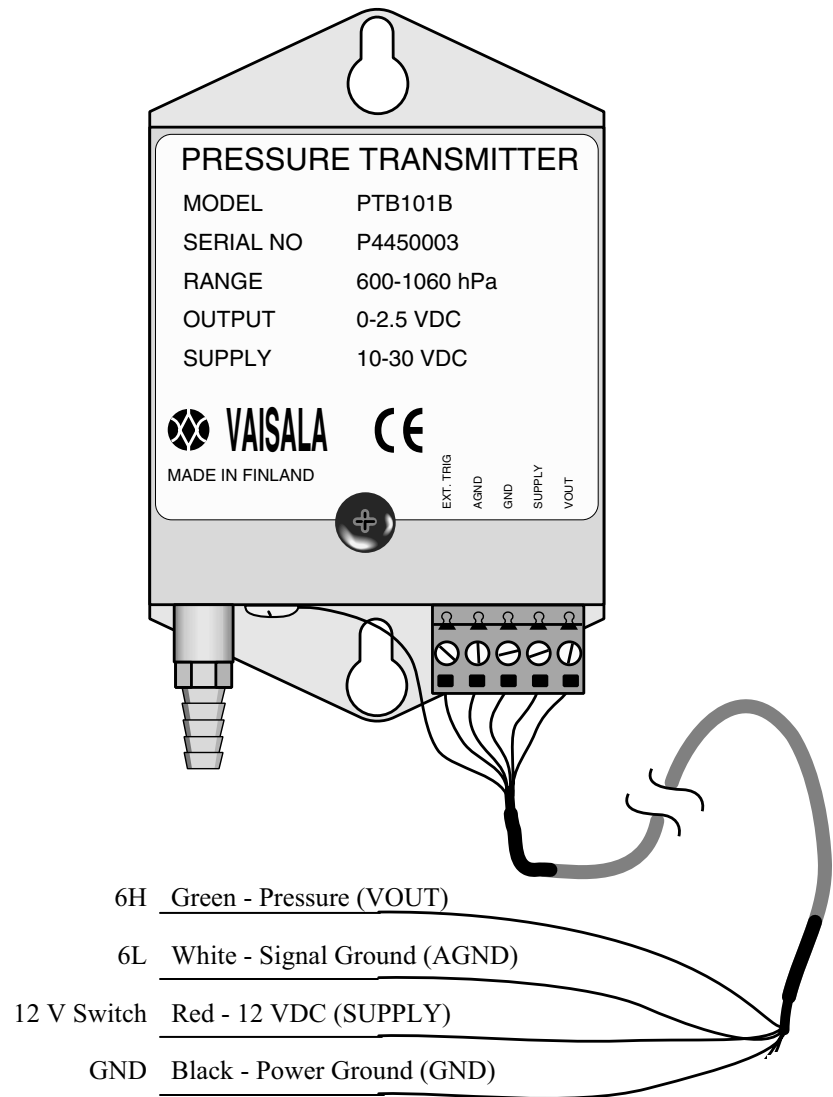


FIGURE 4. CS105MD Wiring Diagram

## 4. Programming

### 4.1 CS105MD

Programming the MetData1 station for the CS105MD is done through Campbell Scientific's Short Cut program. Short Cut includes code in the .DLD file to correct for elevation.

### 4.2 CS105

Atmospheric pressure changes little with time. In most weather station applications measuring pressure once an hour is adequate. In Examples 1 and 2 the datalogger turns on the CS105 one minute before the top of the hour with a control port. As in the example, the execution interval must be one minute or less. On the hour the datalogger measures the CS105, records the pressure, and turns off the CS105.

In Example 3 the CS105 is measured every execution interval. The datalogger turns the CS105 on and waits one second for the CS105 to warm up, before the measurement is made.

The execution interval must be long enough to accommodate the one second delay, to warm up the CS105, and all the other measurement and processing instructions in the program.

In Example 4, the CS105 is measured every execution interval with a 21X. An excitation channel is used to turn the CS105 on and off.

#### WARNING

---

**A CR10(X), CR500, and CR510 excitation channel cannot be used to turn the CS105 on and off because the maximum excitation voltage is 2.5 volts. The CS105 control requires 5 VDC.**

---

In the example programs the pressure is reported in millibars (mb). To report pressure in different units, multiply (Edlog Instruction 37) the measured pressure by the appropriate conversion factor (Table 2).

<b>TABLE 2. Conversion Factors for Alternative Pressure Units</b>	
<b>To Find</b>	<b>Multiply by</b>
kPa	0.1
mm of Hg	0.75006
in of Hg	0.02953
PSI	0.0145

**Example 1. CR1000 Program for Measuring the CS105 Once Every Hour**

```

Main Program
BeginProg
  Scan(5,Sec,1,0)
  'CS105 Barometric Pressure Sensor measurement BP_mmHg:
  If IfTime(59,60,Min) Then PortSet(1,1)
  If IfTime(0,60,Min) Then
    VoltSE(BP_mmHg,1,mV2500,1,1,0,_50Hz,0.184,600.0)
    BP_mmHg=BP_mmHg*0.75006
    PortSet(1,0)
  EndIf
  'Call Data Tables and Store Data
  NextScan
EndProg

```

**Example 2. CR10(X) Program for Measuring the CS105 Once Every Hour**

```

;{CR10X}
;
*Table 1 Program
01: 30      Execution Interval (seconds)

01: If time is (P92)
1: 59      Minutes (Seconds --) into a
2: 60      Interval (same units as above)
3: 41*     Set Port 1* High

02: If time is (P92)
1: 0       Minutes (Seconds --) into a
2: 60      Interval (same units as above)
3: 30      Then Do

03: Volts (SE) (P1)
1: 1       Repts
2: 25**    ± 2500 mV 60 Hz Rejection Range
3: 7*      SE Channel
4: 1*      Loc [ P_mb   ]
5: .184    Mult
6: 600     Offset

04: Do (P86)
1: 51*     Set Port 1* Low

05: End (P95)

06: If time is (P92)
1: 0       Minutes (Seconds --) into a
2: 60      Interval (same units as above)
3: 10      Set Output Flag High (Flag 0)

```

```

07: Real Time (P77)
  1: 0110      Day,Hour/Minute

08: Sample (P70)
  1: 1         Reps
  2: 1*        Loc [ P_mb   ]

-Input Locations-
1 P_mb

* Proper entries will vary with program and datalogger channel, and input location assignments.
** On the 21X use the 5000 mV slow range.
    
```

**Example 3. CR10(X) Program for Measuring the CS105 Every Execution Interval**

```

;{CR10X}
;
*Table 1 Program
  01: 2         Execution Interval (seconds)

01: Do (P86)
  1: 41*        Set Port 1* High

02: Excitation with Delay (P22)
  1: 1         Ex Channel
  2: 0         Delay W/Ex (units = 0.01 sec)
  3: 100       Delay After Ex (units = 0.01 sec)
  4: 0         mV Excitation

03: Volts (SE) (P1)
  1: 1         Reps
  2: 25**      ± 2500 mV 60 Hz Rejection Range
  3: 7*        SE Channel
  4: 1*        Loc [ P_mb   ]
  5: .184      Mult
  6: 600       Offset

04: Do (P86)
  1: 51*        Set Port 1* Low

05: If time is (P92)
  1: 0         Minutes (Seconds --) into a
  2: 30        Interval (same units as above)
  3: 10        Set Output Flag High (Flag 0)

06: Real Time (P77)
  1: 0110      Day,Hour/Minute

07: Average (P71)
  1: 1         Reps
  2: 1*        Loc [ P_mb   ]
    
```

-Input Locations-

1 P\_mb

\* Proper entries will vary with program and datalogger channel, and input location assignments.

\*\* On the 21X use the 5000 mV slow range.

**Example 4. 21X Program for Measuring the CS105 Every Execution Interval Using an Excitation Channel to Turn the CS105 On and Off.**

```

;{21X}
;
*Table 1 Program
  01: 2          Execution Interval (seconds)

01: Excite Delay Volt (SE) (P4)
  1: 1          Reps
  2: 5          SE Channel
  4: 1*         Excite all reps w/Exchan 1
  5: 100        Delay (units 0.01 sec)
  6: 5000       mV Excitation
  7: 1*         Loc [ P_mb   ]
  8: .184       Mult
  9: 600        Offset

02: If time is (P92)
  1: 0          Minutes into a
  2: 30         Minute Interval
  3: 10         Set Output Flag High

03: Real Time (P77)
  1: 0110       Day,Hour/Minute

04: Average (P71)
  1: 1          Reps
  2: 1*         Loc [ P_mb   ]

-Input Locations-
1 P_mb

```

\* Proper entries will vary with program and datalogger channel, and input location assignments.

## 5. Long Lead Lengths

There is a 0.06 mV/foot voltage drop in the CS105 signal leads. This voltage drop, in long lead lengths, will raise the barometric reading by approximately 1.1 mb per 100 feet.

For lead lengths greater than 20 feet, use the differential instruction (Instruction 2) to measure the CS105.

**Example 5. CR10(X) Program for Measuring the CS105 Once Every Hour with Instruction 2 (Differential Measurement)**

```

;{CR10X}
;
*Table 1 Program
  01: 10      Execution Interval (seconds)

01: If time is (P92)
  1: 59      Minutes (Seconds --) into a
  2: 60      Interval (same units as above)
  3: 41*     Set Port 1* High

02: If time is (P92)
  1: 0       Minutes (Seconds --) into a
  2: 60      Interval (same units as above)
  3: 30      Then Do

03: Volt (Diff) (P2)
  1: 1       Reps
  2: 25*     ± 2500 mV 60 Hz Rejection Range
  3: 4*      DIFF Channel
  4: 1*      Loc [ P_mb   ]
  5: .184    Mult
  6: 600     Offset

04: Do (P86)
  1: 51*     Set Port 1* Low

05: End (P95)

06: If time is (P92)
  1: 0       Minutes (Seconds --) into a
  2: 60      Interval (same units as above)
  3: 10      Set Output Flag High (Flag 0)

07: Real Time (P77)
  1: 0110    Day,Hour/Minute

08: Sample (P70)
  1: 1       Reps
  2: 1*      Loc [ P_mb   ]

-Input Locations-
1 P_mb

* Proper entries will vary with program and datalogger channel, and input location assignments.
** On the 21X use the 5000 mV slow range.

```

## 6. Correcting Pressure to Sea Level

The weather service, most airports, radio stations, and television stations reduce the atmospheric pressure to a common reference (sea level). Equation 1 can be used to find the difference in pressure between the sea level and the site. That value ( $dP$ ) is then added to the offset (600 mb) in the measurement instruction. U. S. Standard Atmosphere and dry air were assumed when Equation 1 was derived (Wallace, J. M. and P. V. Hobbes, 1977: *Atmospheric Science: An Introductory Survey*, Academic Press, pp. 59-61).

$$dP = 1013.25 \left\{ 1 - \left( 1 - \frac{E}{44307.69231} \right)^{5.25328} \right\} \quad (1)$$

The value  $dP$  is in millibars and the site elevation,  $E$ , is in meters. Add  $dP$  to the offset in the measurement instruction.

Use Equation (2) to convert from feet to meters.

$$E(m) = \frac{E(ft)}{3.281ft/m} \quad (2)$$

Sea level correction is automatically coded into datalogger programs when using Short Cut.

## 7. Maintenance

There are no user-serviceable parts on CS105. Vaisala recommends recalibrating the CS105 every year. Contact Campbell Scientific, Inc., phone (435) 753-2342, for an RMA number before returning the sensor for recalibration.



# Appendix A. Daily Average

---

If the CS105 will be measured every minute or faster, and a daily average is required, follow Example 5. In Example 5 the daily average, maximum, and minimum pressure is recorded at midnight. A constant is subtracted from the pressure before the average instruction is executed. This prevents the loss of significant digits when adding small numbers to large numbers in floating point arithmetic.

## Example 5. Recording a Daily Average, Maximum, and Minimum Pressure

```
;{CR10X}
;
*Table 1 Program
  01: 5           Execution Interval (seconds)

01: Do (P86)
  1: 41*         Set Port 1* High

02: Excitation with Delay (P22)
  1: 1           Ex Channel
  2: 0           Delay W/Ex (units = 0.01 sec)
  3: 100         Delay After Ex (units = 0.01 sec)
  4: 0           mV Excitation

03: Volts (SE) (P1)
  1: 1           Reps
  2: 25**        ± 2500 mV 60 Hz Rejection Range
  3: 1*          SE Channel
  4: 1*          Loc [ P_mb   ]
  5: .184        Mult
  6: 600         Offset

04: Do (P86)
  1: 51*         Set Port 1 Low*

05: Z=X+F (P34)
  1: 1*          X Loc [ P_mb   ]
  2: -800        F
  3: 2*          Z Loc [ P_const ]

06: If time is (P92)
  1: 0           Minutes (Seconds --) into a
  2: 1440        Interval (same units as above)
  3: 10          Set Output Flag High (Flag 0)

07: Set Active Storage Area (P80)
  1: 3           Input Storage Area
  2: 3*          Loc [ P_mb_avg ]
```

```

08: Average (P71)
  1: 1      Reps
  2: 2*     Loc [ P_const ]

09: If Flag/Port (P91)
  1: 10     Do if Output Flag is High (Flag 0)
  2: 30     Then Do

10: Z=X+F (P34)
  1: 3*     X Loc [ P_mb_avg ]
  2: 800    F
  3: 3*     Z Loc [ P_mb_avg ]

11: End (P95)

12: If time is (P92)
  1: 0      Minutes (Seconds --) into a
  2: 1440   Interval (same units as above)
  3: 10     Set Output Flag High (Flag 0)

13: Set Active Storage Area (P80)
  1: 1      Final Storage Area 1
  2: 10     Array ID

14: Real Time (P77)
  1: 0110   Day,Hour/Minute

15: Sample (P70)
  1: 1      Reps
  2: 3*     Loc [ P_mb_avg ]

16: Maximize (P73)
  1: 1      Reps
  2: 10     Value with Hr-Min
  3: 1*     Loc [ P_mb ]

17: Minimize (P74)
  1: 1      Reps
  2: 10     Value with Hr-Min
  3: 1*     Loc [ P_mb ]

-Input Locations-
1 P_mb
2 P_const
3 P_mb_avg

* Proper entries will vary with program and datalogger channel, and input location assignments.
** With a 21X, use the 5000 mV measurement range.

```



## **Campbell Scientific Companies**

---

### **Campbell Scientific, Inc. (CSI)**

815 West 1800 North  
Logan, Utah 84321  
UNITED STATES  
[www.campbellsci.com](http://www.campbellsci.com)  
[info@campbellsci.com](mailto:info@campbellsci.com)

### **Campbell Scientific Africa Pty. Ltd. (CSAf)**

PO Box 2450  
Somerset West 7129  
SOUTH AFRICA  
[www.csafrica.co.za](http://www.csafrica.co.za)  
[cleroux@csafrica.co.za](mailto:cleroux@csafrica.co.za)

### **Campbell Scientific Australia Pty. Ltd. (CSA)**

PO Box 444  
Thuringowa Central  
QLD 4812 AUSTRALIA  
[www.campbellsci.com.au](http://www.campbellsci.com.au)  
[info@campbellsci.com.au](mailto:info@campbellsci.com.au)

### **Campbell Scientific do Brazil Ltda. (CSB)**

Rua Luisa Crapsi Orsi, 15 Butantã  
CEP: 005543-000 São Paulo SP BRAZIL  
[www.campbellsci.com.br](http://www.campbellsci.com.br)  
[suporte@campbellsci.com.br](mailto:suporte@campbellsci.com.br)

### **Campbell Scientific Canada Corp. (CSC)**

11564 - 149th Street NW  
Edmonton, Alberta T5M 1W7  
CANADA  
[www.campbellsci.ca](http://www.campbellsci.ca)  
[dataloggers@campbellsci.ca](mailto:dataloggers@campbellsci.ca)

### **Campbell Scientific Ltd. (CSL)**

Campbell Park  
80 Hathern Road  
Shepshed, Loughborough LE12 9GX  
UNITED KINGDOM  
[www.campbellsci.co.uk](http://www.campbellsci.co.uk)  
[sales@campbellsci.co.uk](mailto:sales@campbellsci.co.uk)

### **Campbell Scientific Ltd. (France)**

Miniparc du Verger - Bat. H  
1, rue de Terre Neuve - Les Ulis  
91967 COURTABOEUF CEDEX  
FRANCE  
[www.campbellsci.fr](http://www.campbellsci.fr)  
[campbell.scientific@wanadoo.fr](mailto:campbell.scientific@wanadoo.fr)

### **Campbell Scientific Spain, S. L.**

Psg. Font 14, local 8  
08013 Barcelona  
SPAIN  
[www.campbellsci.es](http://www.campbellsci.es)  
[info@campbellsci.es](mailto:info@campbellsci.es)