

INSTRUCTION MANUAL



SC929 RS232 Interface

9/96

Copyright (c) 1996
Campbell Scientific, Inc.

WARRANTY AND ASSISTANCE

This equipment is warranted by CAMPBELL SCIENTIFIC (CANADA) CORP. ("CSC") to be free from defects in materials and workmanship under normal use and service for **twelve (12) months** from date of shipment unless specified otherwise. ***** **Batteries are not warranted.** ***** CSC's obligation under this warranty is limited to repairing or replacing (at CSC's option) defective products. The customer shall assume all costs of removing, reinstalling, and shipping defective products to CSC. CSC will return such products by surface carrier prepaid. This warranty shall not apply to any CSC products which have been subjected to modification, misuse, neglect, accidents of nature, or shipping damage. This warranty is in lieu of all other warranties, expressed or implied, including warranties of merchantability or fitness for a particular purpose. CSC is not liable for special, indirect, incidental, or consequential damages.

Products may not be returned without prior authorization. To obtain a Return Merchandise Authorization (RMA), contact CAMPBELL SCIENTIFIC (CANADA) CORP., at (780) 454-2505. An RMA number will be issued in order to facilitate Repair Personnel in identifying an instrument upon arrival. Please write this number clearly on the outside of the shipping container. Include description of symptoms and all pertinent details.

CAMPBELL SCIENTIFIC (CANADA) CORP. does not accept collect calls.

Non-warranty products returned for repair should be accompanied by a purchase order to cover repair costs.



CAMPBELL SCIENTIFIC
C A N A D A C O R P .

11564 - 149 street - edmonton - alberta - T5M 1W7
tel 780.454.2505 fax 780.454.2655

www.campbellsci.ca

SC929 RS232 INTERFACE

The SC929 temporarily connects a Campbell Scientific battery-powered PC to a datalogger for data retrieval and program transfer. This interface is typically used in remote locations.

1. SPECIFICATIONS

- Operating temperature: -25° C to +50° C
- Power: Powered by datalogger; current consumption typically 8 mA
- Connections: 9-pin male; connects to datalogger
9-pin female; configured as DCE, connects to AT-type portable PC
- Length: 2 m (6 ft.) cable fitted with two 9-pin 'D' connectors
- Weight: 225 g (~8 oz.)

2. APPLICATION

The SC929 provides a two-way conversion between datalogger logic levels (0 V low, 5 V high) and RS232 logic levels (e.g., -8 V low, + 8 V high). It may be used in applications where a battery-powered laptop is taken to the field to communicate with the datalogger (e.g., transfer data or programs, set clock, monitor data, etc.). It provides a neat, single-cable alternative to an SC12 cable, 7026 cable, and an SC32A Interface, but with some differences (see adjoining note).

NOTE:

There are some significant differences between the SC929 and the SC32A:

- The SC929 does not provide opto-isolation. To prevent ground loops, do not use the SC929 with a computer directly connected to power, powered AC, or other ground-referenced power supplies.
- Unlike the SC32A, the SC929 consumes significant levels of power from the datalogger. To avoid unnecessary power drain, disconnect the SC929 from the datalogger serial I/O port when the SC929 is not in use.
- The SC929 does not have the jumper option that is available with the SC32A and in certain situations odd characters may appear on the PC screen. However, this will not affect the correct operation of Campbell Scientific software.

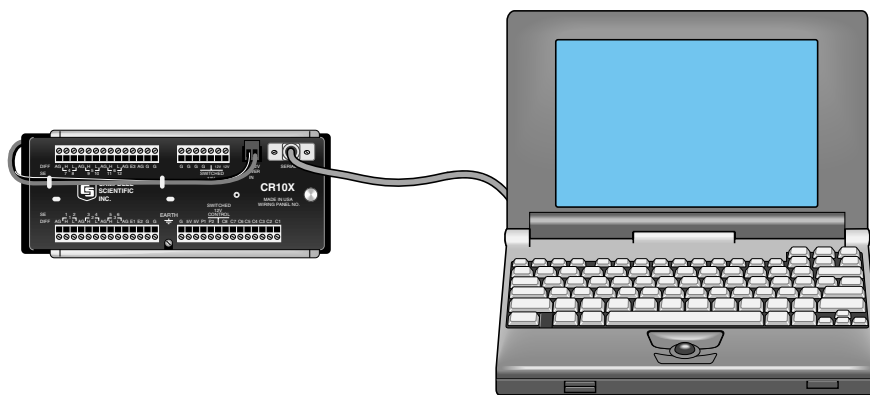


FIGURE 1. The SC929 connects the datalogger's Serial I/O with a laptop's serial port for two-way communication.

SC929 RS232 INTERFACE

Campbell Scientific Companies

Campbell Scientific, Inc. (CSI)

815 West 1800 North
Logan, Utah 84321
UNITED STATES
www.campbellsci.com
info@campbellsci.com

Campbell Scientific Africa Pty. Ltd. (CSAf)

PO Box 2450
Somerset West 7129
SOUTH AFRICA
www.csafrica.co.za
sales@csafrica.co.za

Campbell Scientific Australia Pty. Ltd. (CSA)

PO Box 444
Thuringowa Central
QLD 4812 AUSTRALIA
www.campbellsci.com.au
info@campbellsci.com.au

Campbell Scientific do Brazil Ltda. (CSB)

Rua Luisa Crapsi Orsi, 15 Butantã
CEP: 005543-000 São Paulo SP BRAZIL
www.campbellsci.com.br
suporte@campbellsci.com.br

Campbell Scientific Canada Corp. (CSC)

11564 - 149th Street NW
Edmonton, Alberta T5M 1W7
CANADA
www.campbellsci.ca
dataloggers@campbellsci.ca

Campbell Scientific Ltd. (CSL)

Campbell Park
80 Hathern Road
Shepshed, Loughborough LE12 9GX
UNITED KINGDOM
www.campbellsci.co.uk
sales@campbellsci.co.uk

Campbell Scientific Ltd. (France)

Miniparc du Verger - Bat. H
1, rue de Terre Neuve - Les Ulis
91967 COURTABOEUF CEDEX
FRANCE
www.campbellsci.fr
campbell.scientific@wanadoo.fr

Campbell Scientific Spain, S. L.

Psg. Font 14, local 8
08013 Barcelona
SPAIN
www.campbellsci.es
info@campbellsci.es